NEW APPROACH IN CALIBRATION OF PASSIVE PERMEATION SAMPLERS USED FOR VOC's SAMPLING FROM THE AIR

Monika Partyka, Bożena Zabiegała, Jacek Namieśnik
Department of Analytical Chemistry, Chemical Faculty, Gdańsk
University of Technology
11/12 G. Narutowicza, 80-952 Gdańsk, Poland

7th Passive Sampling Workshop and Symposium RESTON, VA, USA, 24-26.04.2007 1

Mister Chairman Ladies and Gentlemen

First of all I would like to thank the Organizing Committee for this kind invitation to Reston.

It gives me an opportunity to present the new approach in the field of **calibration of passive permeation samplers** used for VOLATILE ORGANIC COMPOUNDS sampling from Indoor Air.




Together with Dr Bozena ZABIEGAŁA we have come from Gdańsk in Poland.

We work at the Chemical Faculty of the Gdańsk University of Technology.



Gdańsk is an Hanzeatic city which in 1997 celebrated its MILLENIUM .

Gdańsk University of Technology is an **old school** founded in 1904.

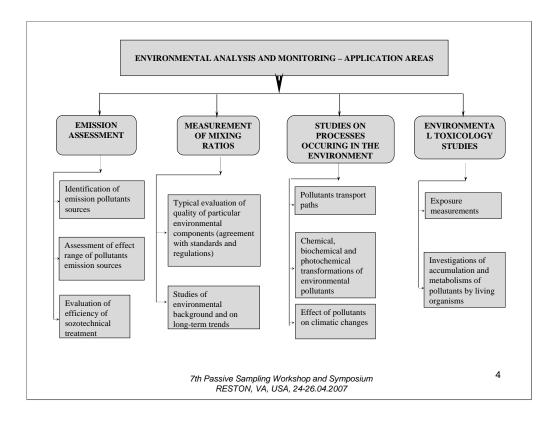

According to more and more common opinion, **analytics and monitoring** of environmental pollutants constitute the **two pillars** on which the entire **environmental science** is based.

There are at least **four goals** of environmental analytics and monitoring.

There are as follows:

- -emission assessment
- **-measurement of mixing ratios** of different types of anthropogenic and biogenic pollutants
- -studies of processes and environmental fate of different xenobiotics
- -ecotoxicological studies.

MAIN CHALLENGES

- low and very low concentration level of analytes
- differences in concentration levels of analytes belonging to the same group/class of compounds
- time and space fluctuations of the analyte concentration
- interferences from other constituents of a sample
- problems with availability of suitable reference materials


7th Passive Sampling Workshop and Symposium RESTON, VA, USA, 24-26.04.2007 5

Main challenges in environmental analytics and monitoring originate from:

- •low and very low concentration level of analytes
- •differences in concentration levels of analytes belonging to the same group/class of compounds
- •time and space fluctuations of analyte concentrations
- •interferences from other constituents of a sample under investigation

problems with availability of suitable reference


materials – needed for validation of analytical procedures and calibration of measuring devices.

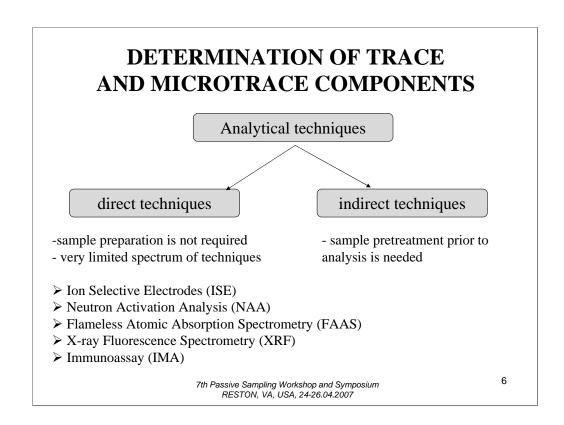

All analytical techniques which can be applied for determination of trace and microtrace components can be divided into two groups:

- -direct techniques- which do not require the sample pretreatment and
- **-indirect techniques-** when specific steps of **sample pretreatment** prior to the final determination of analytes are needed.

Unfortunately, the spectrum of direct techniques is very limited.

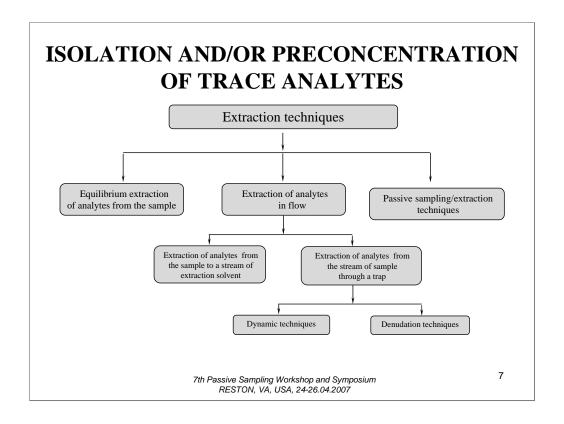


In this situation an additional step of **isolation and preconcentration of analytes** from different matrices has to be introduced to analytical protocols.

These techniques can be divided into three main groups.

It means:

- •Equilibrium extraction of analytes from the sample,
- -Extraction of analytes in flow,
- -Passive extraction techniques known also as passive techniques of sampling the analytes

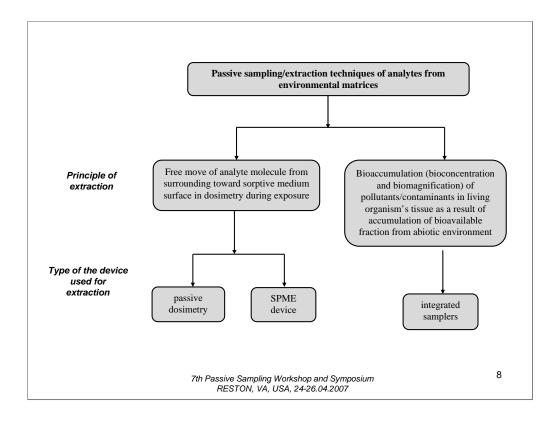


Taking into account variety of methodological approaches and specific designs of passive units, one can propose different classification.

It seems, that the most important bases of classification are:

- -principle of extraction
- -construction of extraction devices.

There is no doubt that passive techniques of extraction of analytes become more and more useful and popular.

I would like to draw your attention to possibility of utilization of living organisms as specific passive samplers.

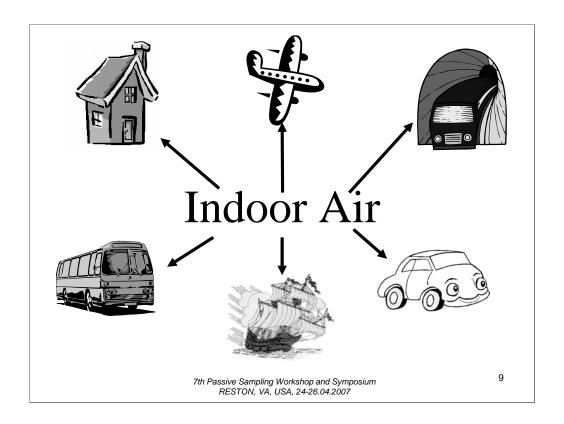

The term 'indoor air" pertains to the air in enclosed environment.


Indoor air means not only air in homes, but also in all places for which regulations concerning workplaces are not applicable.

Indoor air quality is an important parameter, which can affect

-human health

and

-good self-feeling.

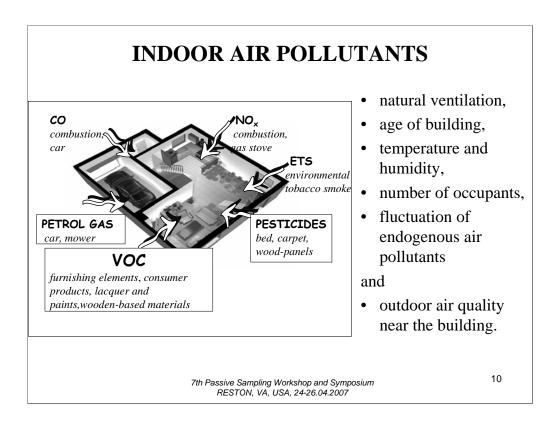

All sources of indoor air pollutants can be divided into two groups:

- -endemic -it means internal sources and
- -external or outdoor sources of emission of pollutants.

WHY DO WE CONTROL INDOOR AIR QUALITY?

- as a response to complaints by room occupants or suspicion that exposure factors that give rise to health concerns are present;
- as a part of a broader epidemiological study;
- assessing effectiveness of intervention;
- need to determine whether specified limits or guideline values are not exceeded.

7th Passive Sampling Workshop and Symposium RESTON, VA, USA, 24-26.04.2007

11

The care for quality of indoor air in present times becomes more and more important.

Taking into account **the amount of time spent by humans indoors**, evaluation of indoor air quality should be as objective as possible.

Indoor air environment investigations may be undertaken for a variety of reasons:

- -as a response to complaints or suspicions that exposure reached dangerous level or
- -as a part of a broader epidemiological study.

Indoor Air Quality is studied also in order to:

- -assess effectiveness of undertaken countermeasures,
- -verify whether specific limits and guidelines are not exceeded.


HOME-MADE PASSIVE SAMPLERS FROM THE DEPARTMENT OF ANALYTICAL CHEMISTRY

- Permeation badge type passive sampler dedicated for air monitoring
- Passive sampler filled with solvent dedicated for aquatic environment

7th Passive Sampling Workshop and Symposium RESTON, VA, USA, 24-26.04.2007 12


Since late 1980's, our research team from the Department of Analytical Chemistry of the Chemical Faculty of Gdansk University of Technology have been involved in application of passive extraction techniques in environmental studies.

We have decided to use a home-made badge-type, passive permeation sampler in order to sample Volatile Organic Compounds from Indoor air.

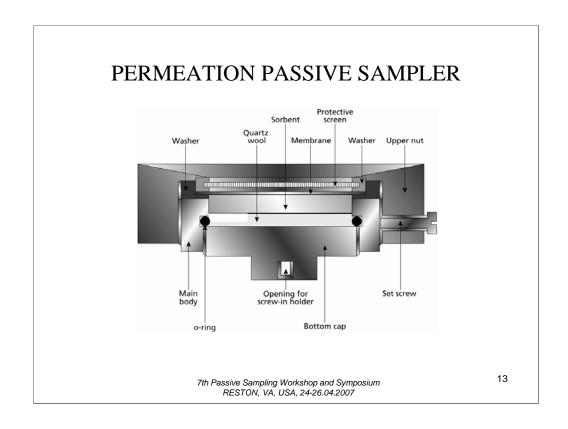


Volatile organic analytes permeate through a membrane and are retained in the active carbon bed.

Membrane made of PDMS foil of 75 micrometer thickness **is the heart** of the sampler.

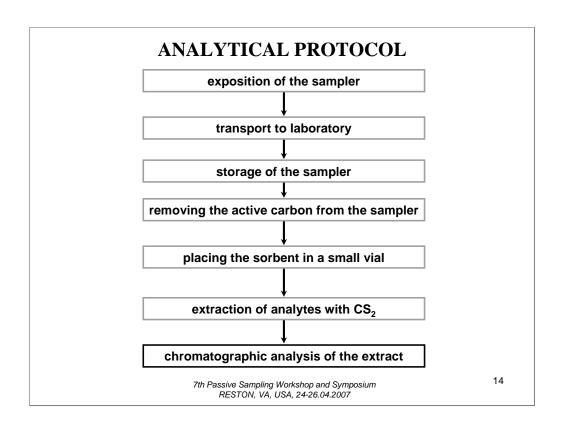

Analytes retained in the sampler are desorbed with CS_2 after the exposure period. Aliquots of extract obtained are subsequently analysed chromatographically.

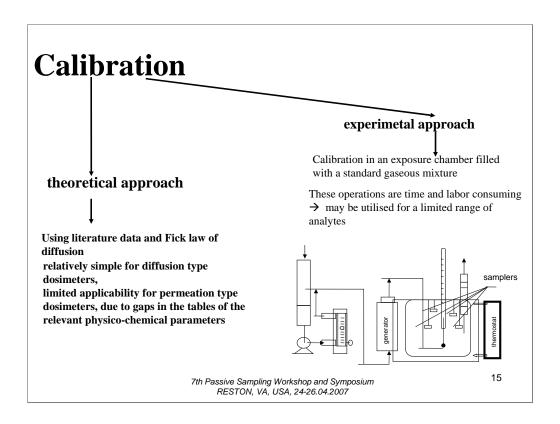

The **main drawback** of the analytical protocols used for determination of VOC's **in indoor air** and based on **application of passive samplers** at the step of sampling the analytes is the NECESSITY of CALIBRATION of new samplers in order to evaluate calibration parameters.

Experimental calibration of set of samplers is a labour - and time consuming task.

The new approach suggested

Evaluation of the calibration parameters on the basis of physico-chemical properties of individual analytes

GOAL:

shortening and simplification of the calibration stage of passive samplers

practical utilisation of the method in real conditions (for monitoring of indoor air quality)

7th Passive Sampling Workshop and Symposium RESTON, VA, USA, 24-26.04.2007 16

Our idea was:

to find **relationships** between **physico-chemical properties** of analytes and their calibration parameters.

PERMEABILITY

 $\boldsymbol{D}_{\boldsymbol{e}}$ - effective diffusion coefficient of the analyte in the membrane material

K - partition coefficient of the analyte between the membrane material and ambient air

 $L_{\rm M}$ – membrane thickness

So far, calibration parameters had to be determined experimentally for <u>each individual analyte</u>

7th Passive Sampling Workshop and Symposium RESTON, VA, USA, 24-26.04.2007 17

Calibration parameters are **compound dependent**, because **permeability** through a membrane depends on:

- -Diffusion of the analyte through the membrane and
- -lts partition between the membrane material and surrounding air.

Due to this, calibration parameters must be determined for each compound individually.

NEW APPROACH

Estimation of the calibration parameters of analytes from specific group on the basis of their physico-chemical properties:

- number of carbon atoms in of a homologous series of compounds
- boiling point
- · molecular weight
- GC retention indices

7th Passive Sampling Workshop and Symposium RESTON, VA, USA, 24-26.04.2007 18


It seems, that it is possible to use, for evaluation of calibration parameters, such **physico-chemical properties** of analytes as:

- the number of carbon atoms in a molecule
- boiling point of a compound
- its molecular weight.

There is also a possibility to assess the **values of calibration constants** on the basis of **GC retention indices**.

One condition must be fulfilled:


- Analytes should belong to the same family, it means to the same homologous series of chemical compounds.

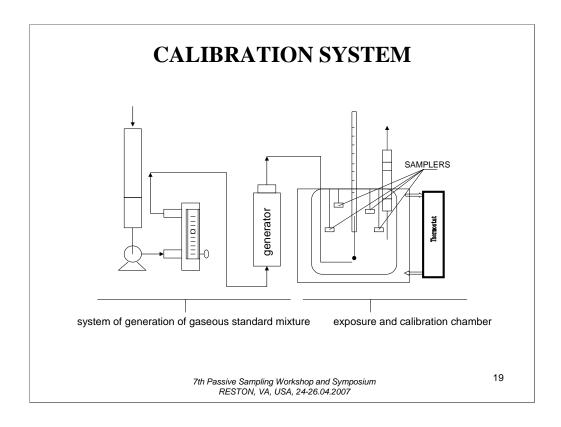


Our system used for experimental calibration of permeation passive samplers consists of:

- -system of generation of gaseous standard mixtures
- -thermostated exposure chamber in which permeation passive samplers are placed.


It seems, that the most suitable source of stream of analytes are permeation tubes placed in the generator.

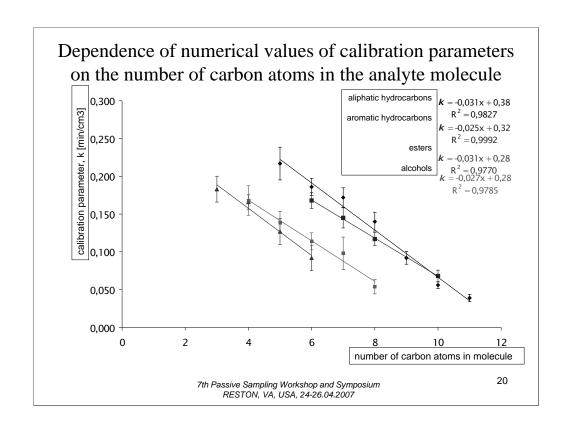


We have found quite a good correlation between **calibration parameters** and the **number of carbon atoms in the analyte molecule**.

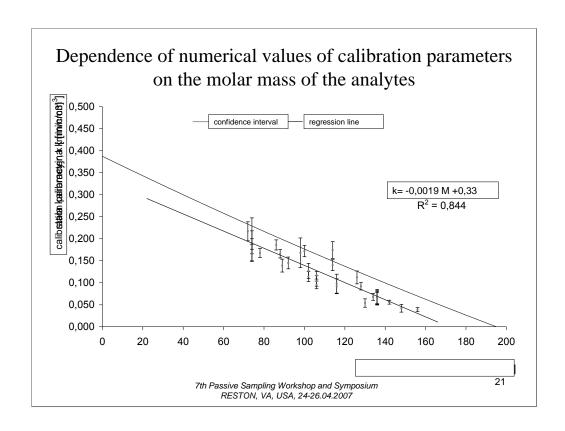

There is also a **very good relationship** between **calibration parameters** and the **molar mass** of the analytes.

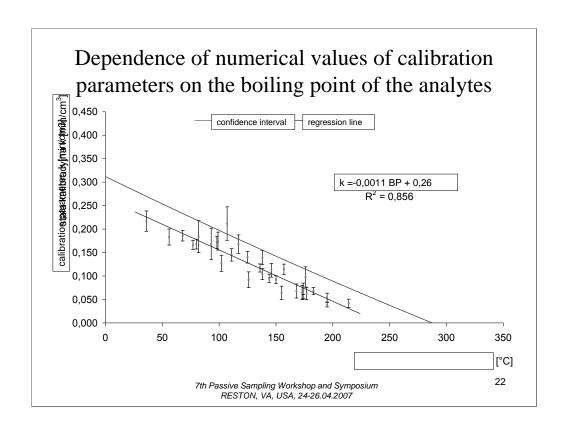


The same type of relationship we have found between calibration parameters and the boiling point of the analytes.

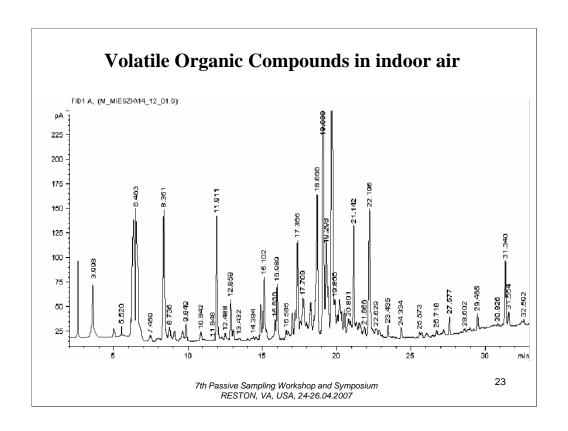

Chromatogram presented in this figure has been obtained during the analysis of sample of analytes retained on sorbent bed in permeation passive sampler.

This chromatogram, will have some analytical value, if all or at least the major peaks will be identified and quantified.

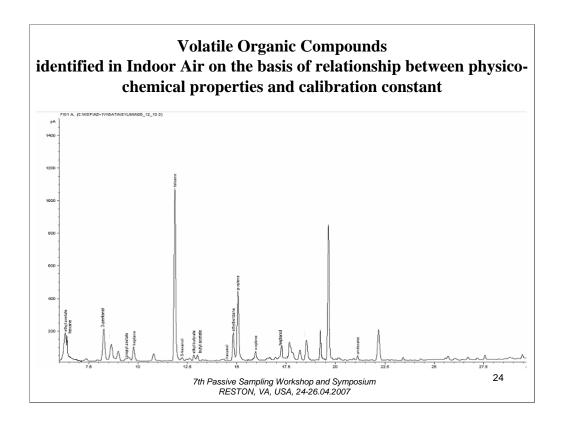

On this chromatogram, I would like to show **volatile organic compounds** present in **indoor air** for which **calibration parameters** have been assessed on the basis of the proposed approach.

There are **14 compounds identified** for which calibration parameters are known.

SYSTEMS OF RETENTION INDICES - LTPRI

$$LTPRI = 100 \cdot \frac{t_A - t_n}{t_{n+1} - t_n} + 100 \cdot n$$

LTPRI – retention index at linear temperature program (linearly increasing temperature of chromatographic column) of a given analyte

t_A – retention time of this analyte

t_n - retention time of n-alkane eluted directly before this analyte

 t_{n+1} – retention time of n-alkane eluted directly after this analyte

 $\ensuremath{n}-\ensuremath{n}\xspace$ number of carbon atoms in a moilecule of n-alkane eluted directly before this analyte

7th Passive Sampling Workshop and Symposium RESTON, VA, USA, 24-26.04.2007 25

We have also decided to verify the possibility of use of system **of retention indices** to facilitate the step of calibration of passive permeation samplers.

LTPRI system is based on KOVATS RETENTION INDICES.

This system was proposed in 1963.

LTPRI system and calibration parameters

- Permeability through the membrane is determined primarily by the solubility of the analyte in the membrane material
- The membrane is made of the same material as the stationary phase in the GC column used (PDMS)
- Retention time is determined by the partition coefficient of the analyte between the carrier gas and the stationary phase, which also depends on the solubility of the analyte in PDMS

A relationship between the retention parameters and the calibration constants of the analytes should be observed!

7th Passive Sampling Workshop and Symposium RESTON, VA, USA, 24-26.04.2007

26

There should be a **relationship** between the **retention parameters** and the **calibration constants** of analytes.

This **statement** is connected with the fact, that **retention time** is **controlled** by the **partition coefficient** of the analyte between the carrier gas and the stationary phase in chromatographic column.


LTPRI

Values of LTPRI have been determined:


- ✓ at different chromatographic conditions:
 - ***** carrier gas flow-rate,
 - * temperature-in-time gradient,
 - * initial column temperature.
- ✓ using capillary columns from different manufacturers (Agilent, Quadrex, J&W, Resteck)
- ✓ different GC models (HP 5890, HP 6890, Perkin-Elmer XL AS)

7th Passive Sampling Workshop and Symposium RESTON, VA, USA, 24-26.04.2007 27

Numerical values of LTPRI for a **wide group of analytes** have been determined at different **chromatographic conditions**.

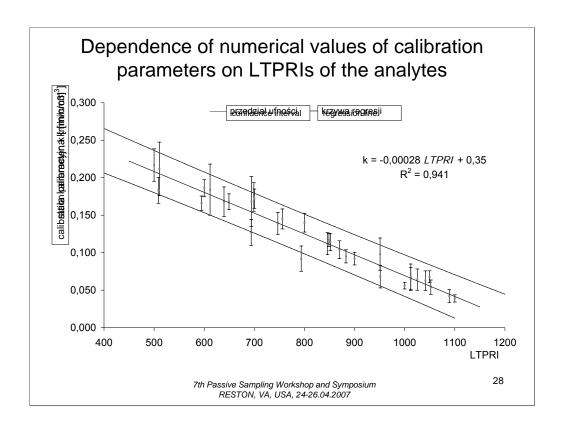

Finally we have **found quite a good correlation** between **calibration constant** of our passive sampler and **LTPRI values**.

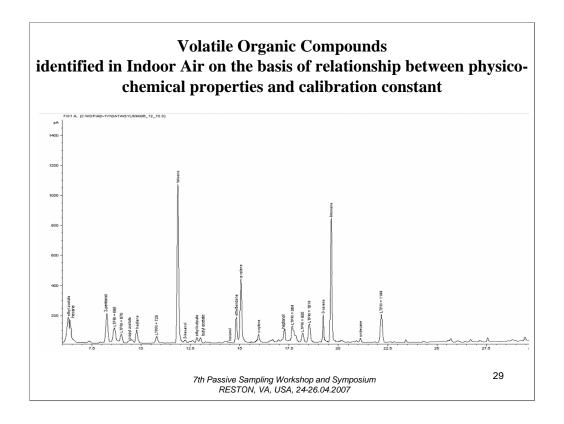

With the use of **linear temperature programmed retention indices approach** we can estimate calibration constants values for all compounds, which are presented on the chromatogram.

There are 24 volatile organic compounds identified with calibration constants evaluated on the basis of LTPRI approach.

There were only 14 compounds identified on the basis of the first approach, it means when physicochemical properties of analytes belonging to the same homologous series are taken into consideration.

MONITORING INDOOR AIR QUALITY

22 apartments (November 2004 – July 2006)

	average	maximum	minimum
Age of apartments [years]	28	101	0
Number of occupants	3	8	1
Living area [m ²]	68	180	26

7th Passive Sampling Workshop and Symposium RESTON, VA, USA, 24-26.04.2007 30


It is high time to tell some words about the application of our samplers in analytical practice.

We have studied the level of concentration of VOLATILE ORGANIC COMPOUNDS in 22 selected dwellings within the TRICITY area.

Tricity is a urban agglomeration composed of Gdansk, Gdynia and Sopot and situated on the southern Baltic Sea coast.

Studies were carried out in period since November 2004 till July 2006.

After the exposure samplers have been transported to laboratory.

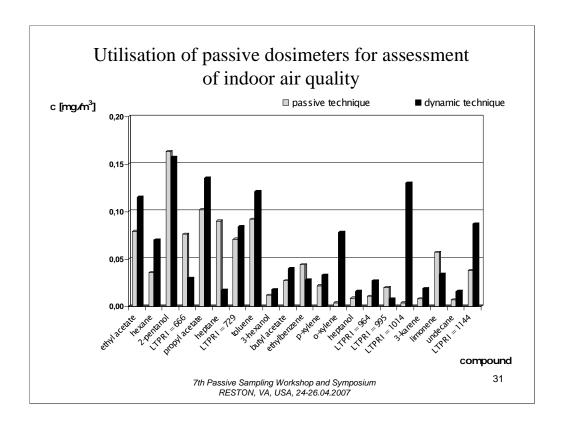

Dynamic technique based on application of:

- -Suitable pump,
- -Flowmeter
- -Sorbent tube

has been used as a REFERENCE technique of **sampling the analytes** from indoor air.

It is worthy to remember that **analytical protocol** carried out in **laboratory** is the **same for both techniques** of sampling the analytes.

TOTAL VOLATILE ORGANIC COMPOUNDS


Total Volatile Organic Compounds (TVOC): a measure representing the sum of all VOCs present in the air to provide an approximate indication of pollutant levels.

Indoor air typically contains hundreds of different VOCs in very low concentrations, some of which can have additive effects.

7th Passive Sampling Workshop and Symposium RESTON, VA, USA, 24-26.04.2007 32

Very often on the basis of analytical results, the value of **Total Volatile Organic Compounds** (TVOC's) is calculated.

This parameter is useful in practice and can be used for the **preliminary** classification of quality of indoor air in different enclosed environment.

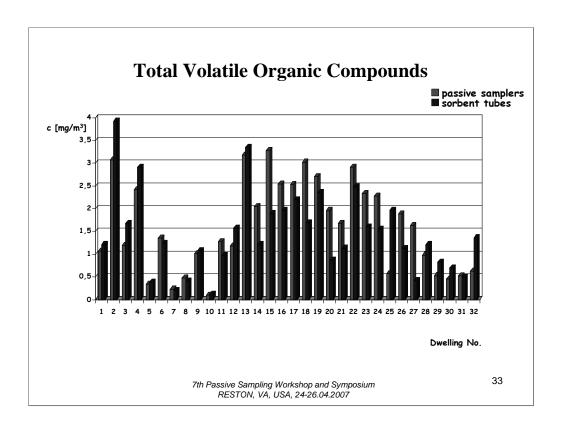

I would like to show you the comparison of the results of determination of **Total Volatile Organic Compounds** in 32 selected **Tricity dwellings**.

Generally no significant differences between **passive and dynamic sampling techniques** were observed.

CONCLUSION

The approach proposed eliminates the biggest obstacle to wider acceptance of permeation passive samplers i.e., the need to calibrate each sampler for each individual analyte

All the advantages of passive sampling remain

Permeation passive samplers can be deployed in the same way as active samplers, i.e. without the need to calibrate them before measurements

> 7th Passive Sampling Workshop and Symposium RESTON, VA, USA, 24-26.04.2007

34

The approach proposed in this presentation **allows to eliminate** fundamental **limitation** of **permeation passive sampling**.

It is possible to estimate the values of the calibration constants on the basis of:

- -physico-chemical properties of the analytes and/or
- -their GC retention parameters.

LITERATURE

- NamieŚnik J., Górecki T., *LC-GC Europe*, **13**, 2000, 678.
- Zabiegała B., Zygmunt B., Przyk E., NamieŚnik J., *Anal. Lett.*, **33**, 2000, 1361.
- Zabiegała B., Przyk E., Przyjazny A., NamieŚnik J., *Chem. Anal.*, **45**, 2000, 11.
- Przyk E., Zabiegała B., Górecki T., Namieśnik J., *Chem. Anal.*, **45**, 2000, 631.
- Zabiegała B., Kot A., NamieŚnik J., *Chem. Anal.*, **45**, 2000, 645.
- Górecki T., NamieŚnik J., TrAC., 21, 2002, 276.
- Zabiegała B., Górecki T., Przyk E., Namieśnik J., Atmos. Environ., 36, 2002, 2907.
- Zabiegała B., Górecki T., NamieŚnik J., Anal. Chem., 75, 2003, 3182.
- NamieŚnik J., Zabiegała B., Kot-Wasik A., Partyka M., Wasik A., *Anal Bioanal Chem*, **381**, 2005, 279.

http://www.pg.gda.pl/chem/Katedry/Analityczna

7th Passive Sampling Workshop and Symposium RESTON, VA, USA, 24-26.04.2007

35

We think that this **new approach** in the field of **calibration of passive dosimeters will simplify analytical work** and make it possible to **apply passive dosimeters** on a larger scale.

More information on our research you can find in our publications.


The whole list is easily **accessible on homepage** of the Department of Analytical Chemistry.

Please, do not hesitate to contact me during this conference or later by e-mail.



I would like to inform you that the 35th International symposium on Environmental Analytical Chemistry will take place in Gdansk in 2008.

As the Chairman of the Organizing Committee I have a pleasure to invite you. YOU ARE WELCOME!

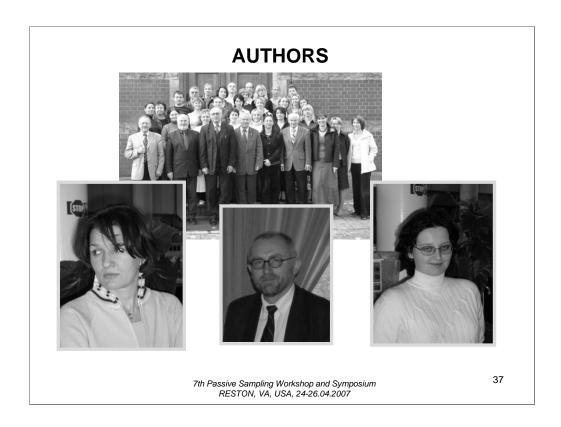

Finally, I would like to introduce to you

the whole team from my Department of Analytical Chemistry and coauthors of this presentation:

- -dr Bożena ZABIEGAŁA, who is present here
- dr Monika PARTYKA **who carried out the major part of these studies** as her PhD thesis.

THANK YOU FOR YOUR ATTENTION

7th Passive Sampling Workshop and Symposium RESTON, VA, USA, 24-26.04.2007 38